

Analysis of Surface Microdefects Localization Possibilities

V. Bulbenkienė

*Department of Informatics Engineering, Klaipėda University,
Bijūnų str. 17, LT-91225, Klaipėda, Lithuania, phone: +370 46 398986, e-mail: violeta.bulbenkiene@ik.ku.lt*

R. Pūras

*Institute of Material Science and Applied Research, Vilnius University,
Saulėtekio av. 9-III, LT-10222, Vilnius, Lithuania, phone: +370 5 2366096, e-mail: romualdas.puras@ff.vu.lt*

S. Sakalauskas

*Department of Semiconductor Physics, Vilnius University,
Saulėtekio av. 9-III, LT-10222, Vilnius, Lithuania, phone: +370 5 2366029, e-mail: stanislavas.sakalauskas@ff.vu.lt*

Introduction

Adsorption phenomenon as well as surface structure variation of samples, especially semiconductors, calls significant electron work function variation. Well-known methods of electron work function measurement, such as photoelectric and thermoelectronic, yield to of Kelvin–Zisman vibrating probe method by properties. The latter method is the best approbated and is characterized by the highest sensitivity in surface physics [1, 2]. This method is realized by various measuring instruments which spatial resolution mainly is determined by the diameter of vibrating probe and reaches about hundred nanometers. Subsequent reduction of vibrating probe tip's diameter can change converter working conditions from quasioleostatic to tunnel therefore we will not analyze it. Else, all measurement systems are inert, i.e. their frequency pass band is limited, so even analysis of small surface area requires some time [3], for instance analysis of 1 mm² area with 1 μm spatial resolution runs around (10⁴ ... 10⁶) s, i. e. from 0.11 to 11 days.

Usually surface microdefects cover small part of real structure surface under investigation therefore vibrating probe with tip's diameter considerably higher than the area of possible microdefect can be used for rapid control. However by which indication it is possible to localize such microdefect. The aim of this work was to investigate the possibilities localization of microdefect or microdefect's group when the diameter of vibrating probe tip's is noticeable higher the dimension of microdefect.

Scanning speed of samples surface

Simplified model of Kelvin–Zisman converter and sample under investigation is shown in Fig. 1. Vibrating

electrode 1 and surface of investigating sample form periodically alternating, i. e. parametric, capacity $C(t) = C_0 [1 + (\Delta C/C_0) \cos \omega t]^{-1}$. Electric charge of the capacity is proportional to difference of electron work functions, i. e. $Q(t) = C(t)(A_1 - A_2)q^{-1}$, here q – electron charge. If we choose high nominal resistor R to warranty $RC_0\omega \gg 1$, we will have voltage signal of the frequency ω , the amplitude of which is proportional to difference of electron work functions. This is informative signal, which is gained and detected later.

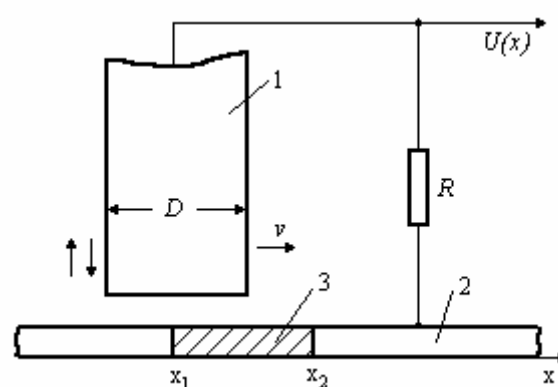


Fig. 1. Model of vibrating electrode (1) and surface of sample under investigation (2). 3 – defective area which diameter is $x_2 - x_1 = D$, v – speed of electrode shift (scanning)

According to theoretical analysis and experimental study the threshold linear resolution of this method is determined by dimension of vibrating electrode tip, when distance between the tip and sample surface is significantly

less the dimension of the tip and also if electronic equipment has infinite frequency pass band. It is necessary to accept appropriate transfer characteristics of equipment (Fig. 2) for more precise estimation of scanning speed. The nature of the characteristic depends on the vibrating electrode tip area and geometry of the informative surface area: square-strip (1), circle-strip (2), circle-circle (3). There are few papers [4, 5] analyzing vibrating probe scanning speed and results are close to ours but authors didn't present an analysis of optimal scanning speed, its dependence on the dimension of the vibrating probe and the frequency pass band of the electronic system.

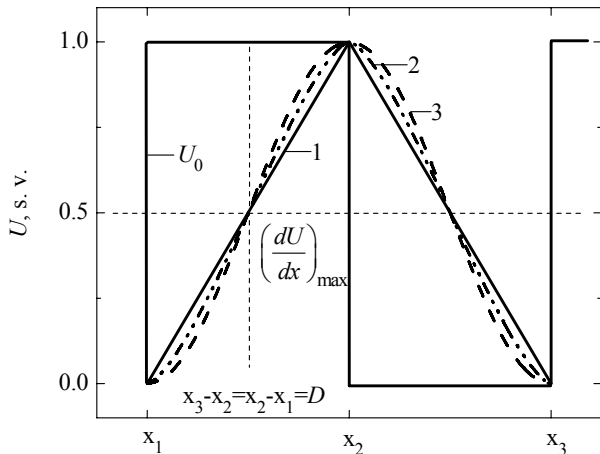


Fig. 2. Accepted character of surface potential U_0 , which characterizes the informative area and the measured potential, when the electrode's tip and informative area are such: square-strip (1), circle-strip (2), circle-circle (3).

In practice the last, i. e. third, case (or close to that) commonly takes place. We prefer this case because the output signal may be precisely and simply described as follows: $U(x) = U_0 \sin^2 ax$. Even in an ideal case the output voltage is shifted towards the vibrating electrode movement. In this case the coordinate of the center of the defective area may be determined by the maximal value of the derivative, i. e.

$$\left(\frac{dU}{dt}\right)_{\max} \sim \left(\frac{dU}{dx}\right)_{\max} \sim (\sin 2ax)_{\max} \quad \text{in assumption}$$

fixed speed of electrode shift. The vibration frequency of a real size electrode is adjusted in the range of some kHz because at higher frequency the combinative modes can easily form and reduce the operating conditions of the converter. Thus, estimating the low frequency filter's time constant we state that the frequency pass band of such converter will not exceed some hundred Hz. If we will ignore the narrow frequency pass band and will select scanning speed free, we can obtain inadmissible uncertainties of surface potential and its coordinate. Figure 3 shows the theoretical dependencies of the relative error of voltage determination and defective area center's coordinate determination on scanning speed. The scanning speed is expressed as a part of the maximal speed defined by the ratio of the vibrating probe diameter D to the measuring device's time constant τ [3]. According to Fig. 3, the uncertainty of the defective area center's coordinate determination grows faster than the uncertainty of this area

surface electric potential's when scanning speed increases. Therefore, the main attention must be kept to the accuracy of coordinate determination when we select the value of scanning speed. In practice, an acceptable scanning speed may be $(0.01 \dots 0.03)v_m$. In this case, the maximum error of defective center coordinate determination will not exceed 3% and surface potential – 0.5%. These dependencies were qualitatively validated in experiment. It is important to select an appropriate (not high) scanning speed in the study of microdefective areas, which dimensions are considerably less than the diameter of the vibrating probe.

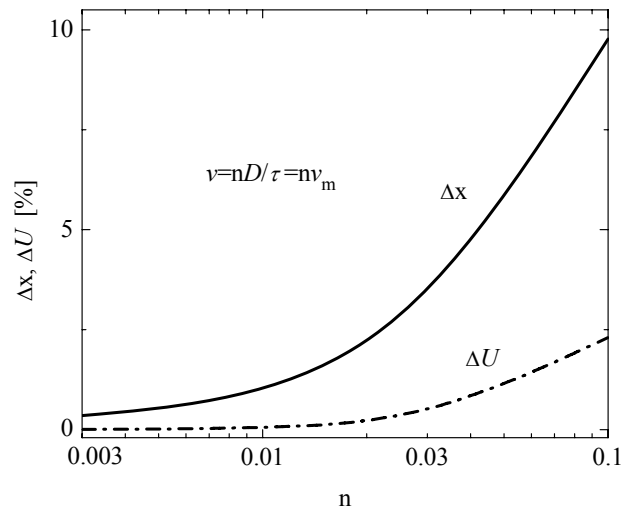


Fig. 3. The theoretical dependencies of the relative error of voltage determination and defective area center's coordinate determination on scanning speed. Scanning speed is expressed as a part of the maximal speed $v_m = D/\tau$ (τ – time constant of the measuring device).

Method localization of surface microdefects

Analyzing the possibilities of localization of surface microdefects, we will have in mind the model presented in Fig. 1, in which the defective area width (or diameter) is far less than the diameter of the vibrating probe, i. e. $x_2 - x_1 \ll D$. It seems as a simply quasi-electrostatic system, but its correct analysis is very complex as follows by the investigation of V. P. Pronin [7]. We preferred experimental investigation.

We had used a 7.5 mm diameter vibrating probe to warrant sufficient measurement accuracy. The diameter of the constructed defective area ($x_2 - x_1$) was 1 mm and the distance between the electrode tip and sample with the defective area was 1 mm. The time constant of the measuring device was 0.1 s. Scanning speed equal to $0.01D/\tau = 0.75$ mm/s was fixed in experiment. Such scanning speed warranted low measurement uncertainty according to Fig. 3. Experimental results of the investigation of surface electric potential are presented in Fig. 4. It is possible in an unambiguous way to establish the coordinate of the defective area, whereas the center of the defective area's by the derivative maximum of the signal leading edge according to these results. The derivative maximum often coincides with the middle of the leading edge. The time constant of the leading edge cannot be shorter than $(3 \dots 5)\tau$ after experimental results even if the defective area is characterized by a δ -function, i. e. $(x_2 - x_1) \rightarrow 0$. If we ignore this fact we

will have large errors in establishment of defective area coordinate. So we must noticeably reduce scanning speed when we record signal with time constant of leading edge close or shorter to 5τ . In general we state that with

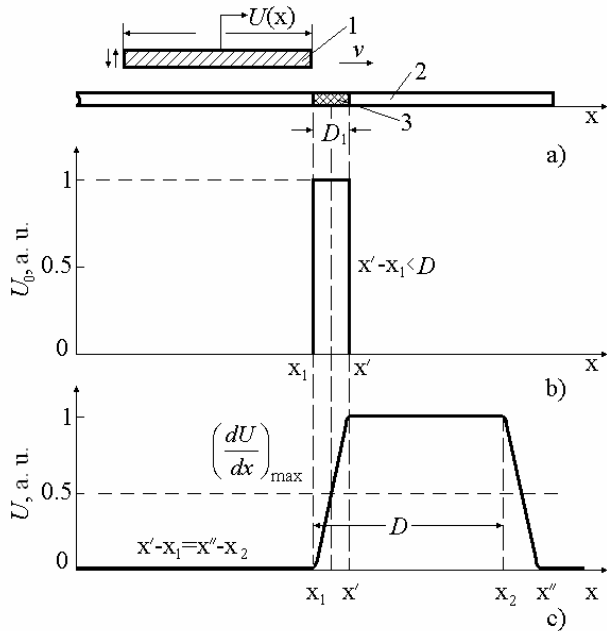


Fig. 4. Accepted model of defective area (a), constructed surface electric potential (b) and measured electric potential (c). Defective area's size is less the diameter of vibrating probe and $U_0 \gg U$.

scanning speed $v=0.01D/\tau$ we will easy measure surface potential and will straight establish coordinate of defective area if width or diameter of this area will be larger than $0.1D$, i. e. $x_2 - x_1 \geq 0.1D$.

Still we had analyzed defective area linear dimension and transition process of signals registered by measuring device assuming signal amplitudes noticeably higher noise voltage. In experiments it was always satisfied. Our surface electric potential measuring device has 100 % negative feedback, which enlarged measurement accuracy and measured voltage value coincided to sample's voltage. It is true if size of informative area is greater the size of vibrating probe. Now we are analyzing case when informative area is noticeably less the area of the tip vibrating electrode and the value of registered voltage will be much less the potential of informative area. It was experimentally established that measured voltage value U is related to defective area potential by relation:

$$U \approx U_0 D^2 / d^2, \quad (1)$$

where $d=x_2-x_1$ (assuming profile of defective area as circle), so measured voltage is low, therefore it is necessary to give attention to the noise voltage.

We would like demonstrate experimental results (Fig. 5) dealing with the same vibrating electrode ($D=7.5$ mm) and defective area was simulated by three circular shape areas with diameter 1 mm and distance between areas 2 mm. According to experimental results it is possible to detect defective areas with area noticeably less the area of vibrating probe tip. Analogous measurements were carried out with vibrating electrode

which tip diameter was 10 μm . Due to insufficient accuracy of scanning device it is possible to compare only qualitatively these results.

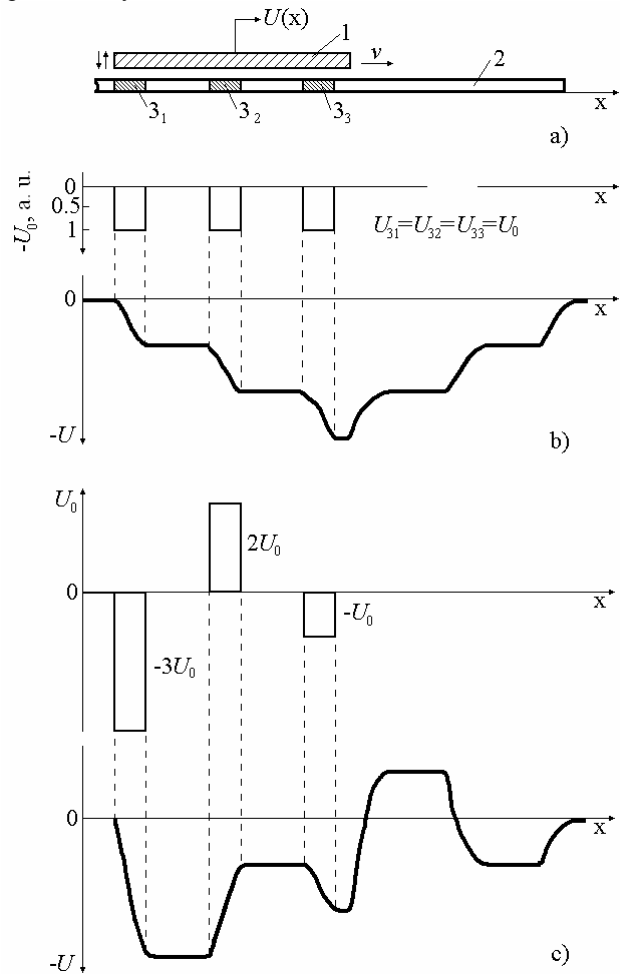


Fig. 5. Constructed experimental model of some defective areas (a) and measured surface electric potential when potential of defective areas are equal and same sign (b) or different values and signs (c). Potential of defective area is far greater than measured.

Conclusions

Analysis of theoretical results and carried out experiments on real samples and its models allows us state that contactless capacitive electric potential measuring devices operating on principle vibrating Kelvin Zisman probe allows:

- to localize single microdefects its groups when their dimensions are less the diameter of vibrating probe;
- approximately measure surface electric potential and jointly electron work function of these microdefective area;
- full-automatic of measuring process with computer analysis and processing of results.

References

1. Lüth H. Surfaces and interfaces of solid materials, Berlin: Springer. –1997. – 556 p.
2. Dai G., Pohlentz F., Danzebrink H. U., Xu M., Hasche K., and Wilkening G. Metrological Large Range Scanning

- Probe Microscope // Review of Scientific Instruments. – 2004. Vol. 75, No. 4. –P. 962–969.
3. **Žilinskas P. J. Lozovski T., and Sakalauskas S.** Features of Non Contact Surface Electrical Potential Measurement Instruments and Applications // Measurements. –2003. – No. 4(28). – P. 11–16.
 4. **Baumgärtner H. and Liess H. D. G.** Micro Kelvin Probe For Local Work-Function Measurements // Review of Scientific Instruments. – 1988. Vol. 59, No. 5. – P. 802–805
 5. **McMurray H. N. and Williams G.** Probe Diameter and Probe-Specimen Distance Dependence in the Lateral Resolution of a Scanning Kelvin Probe // Journal of Applied Physics. – 2002. – Vol. 91, No. 3. – P. 1673–1679.
 6. **Sakalauskas S., Vaitonis Z., and Pūras R.** Method of Microelectronic Charge Converter's Sensitivity Enlargement // Electronics and Electrical Engineering. – 2005. – No. 1(57). – P. 71–73.
 7. **Pronin V. P.** Elektroemkostnyje Sistemy v Elektrofizike, Saratov: Akademija. – 1996. – 312 c. (in Russian)

Submitted 2006 03 23

V. Bulbenkienė, R. Pūras, S. Sakalauskas. Analysis of Surface Microdefects Lokalization Possibilities // Electronics and Electrical Engineering. – Kaunas: Technologija, 2006. –No. 6(70).– P. 87–90.

Analysis of linear spatial resolution of vibrating Kelvin-Zisman electrode is carried out in case when the size of defective area is substantially less than diameter of vibrating probe. Dependence of relative error of voltage determination and defective area center's coordinate determination on scanning speed was examined and influence of measuring device pass band was estimated also. Analysis of theoretical results and carried out experiments on real samples and its models allows us to state that contactless capacitive electric potential measuring devices operating on principle of vibrating Kelvin Zisman probe allows to localize single microdefects and its groups when their dimensions are less the diameter of vibrating probe, approximately measure surface electric potential and electron work function of these microdefective areas. Ill. 5, bibl. 7 (in English; summaries in English, Russian and Lithuanian).

В. Булбенкене, Р. Пурас, С. Сакалаускас. Анализ возможностей локализации поверхностных микродефектов //Электроника и электротехника. – Каунас: Технология, 2006. – № 6(70). – С. 87–90.

Проведен анализ линейной разрешающей способности метода вибрирующего зонда Кельвина-Зисмана, когда размер исследуемой дефектной поверхности намного превышает диаметр вибрирующего зонда. Исследовано влияние скорости сканирования на неопределенность измерения поверхностного электрического потенциала дефектной области и координаты дефектной области, оценено влияние полосы пропускаемых частот измерителя. Анализ теоретических результатов и проведенные эксперименты позволяют делать вывод, что емкостным измерителем поверхностного электрического потенциала можно локализовать отдельные микродефекты и области их групп, когда геометрические размеры таких групп намного меньше диаметра вершины вибрирующего зонда, приблизительно установить поверхностный электрический потенциал этих областей и работу выхода электронов Ил. 5, библи. 7 (на английском языке; рефераты на английском, русском и литовском яз.).

V. Bulbenkienė, R. Pūras, S. Sakalauskas. Paviršinių mikrodefektų lokalizavimo galimybių tyrimas // Elektronika ir elektrotechnika. – Kaunas: Technologija, 2006. – Nr. 6(70).– P. 87–90.

Išanalizuota virpančiojo Kelvino ir Zismano elektrodo metodo linijinė skiriamoji geba, kai tiriamos defektinės srities matmenys yra gerokai mažesni už elektrodo skersmenį. Išnagrinėta defektinės srities paviršinio potencialo ir jos koordinatės matavimo neapibrėžties priklausomybė nuo žvalgos greičio, įvertinta keitiklio praleidžiamų dažnių juostos įtaka. Teorinių rezultatų analizė, atlikti eksperimentiniai tyrimai su realiais bandiniais įgalina tvirtinti, kad talpiniai paviršinio potencialo matavimai leidžia lokalizuoti pavienių mikrodefektų ir jų grupių sritis, kai tų sričių geometriniai matmenys kur kas mažesni už virpančiojo elektrodo viršūnės skersmenį, apytiksliai nustatyti šių mikrodefektinių sričių paviršinių elektrinių potencialą ir išlaisvinimo darbo vertę. Il. 5, bibl. 7 (anglų kalba; santraukos anglų, rusų ir lietuvių k.).

